



Fig. 2

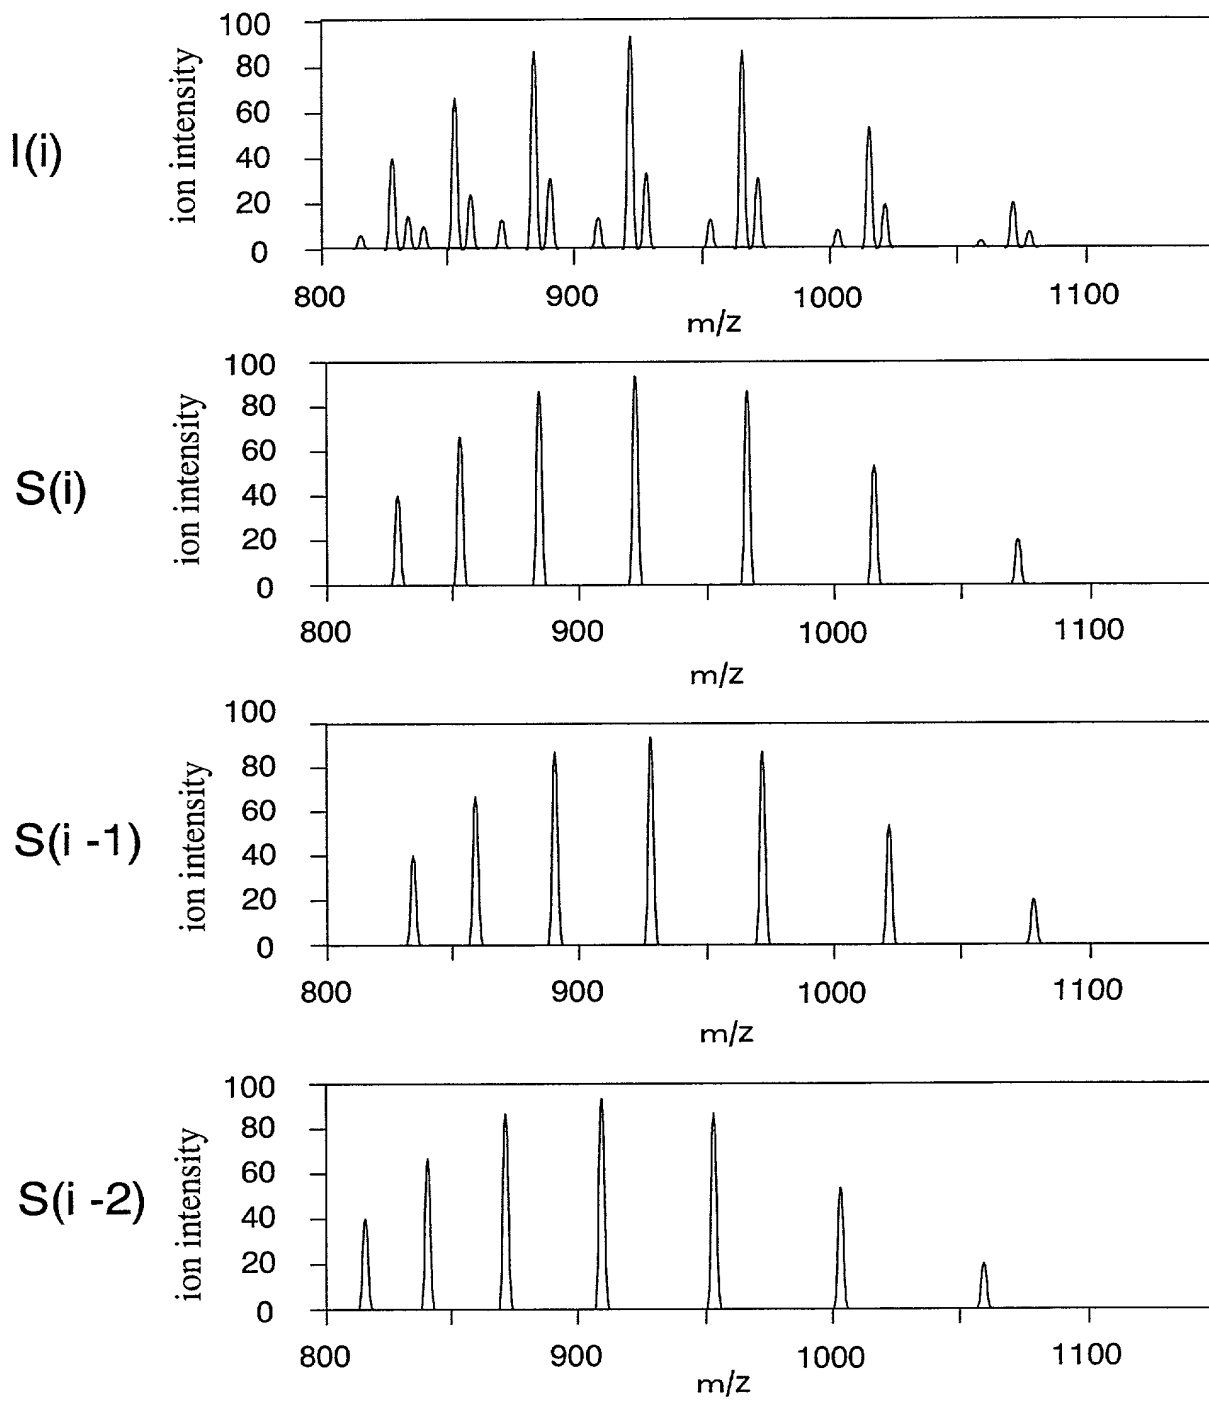


Fig. 3

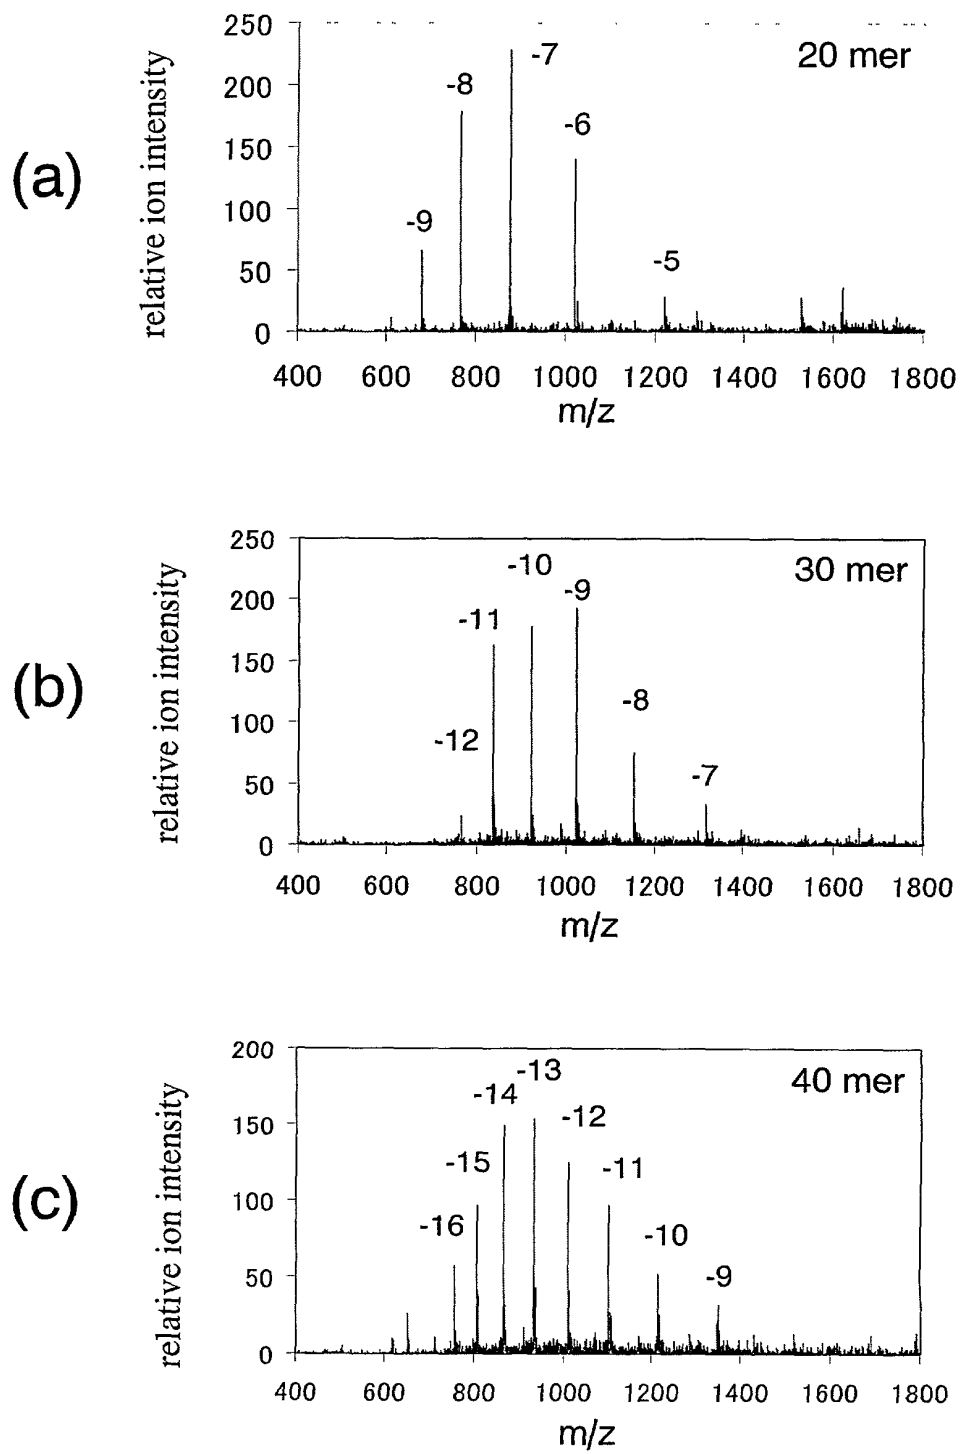


Fig. 4

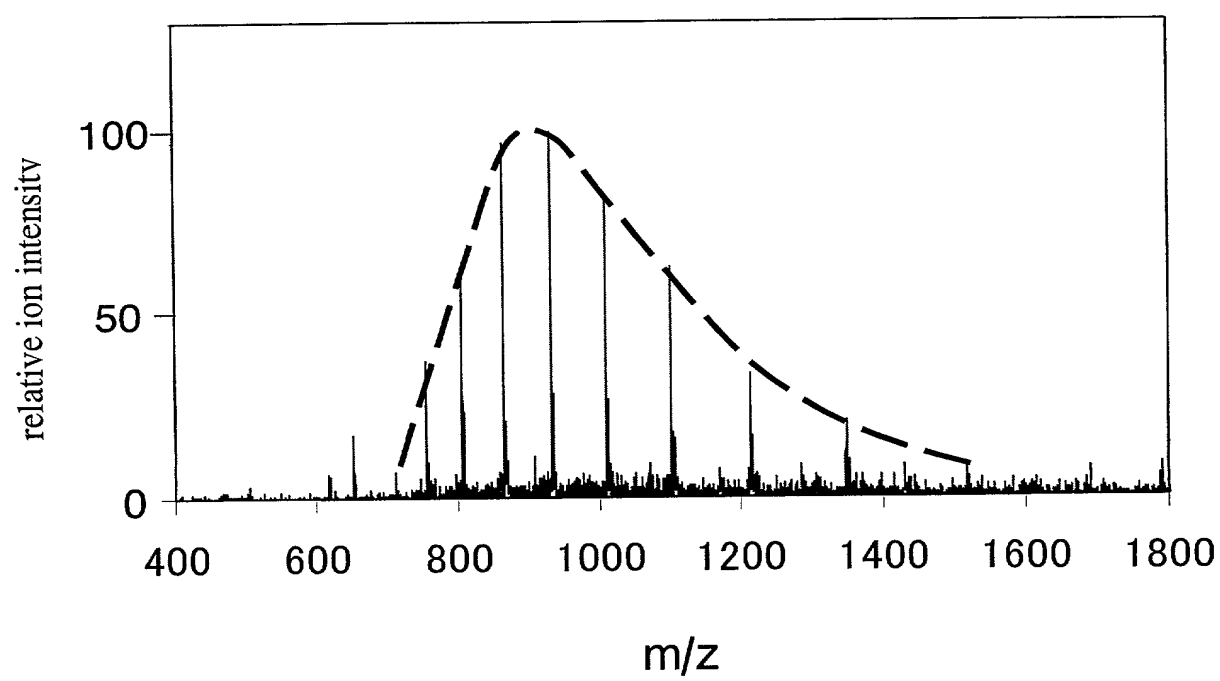


Fig. 5

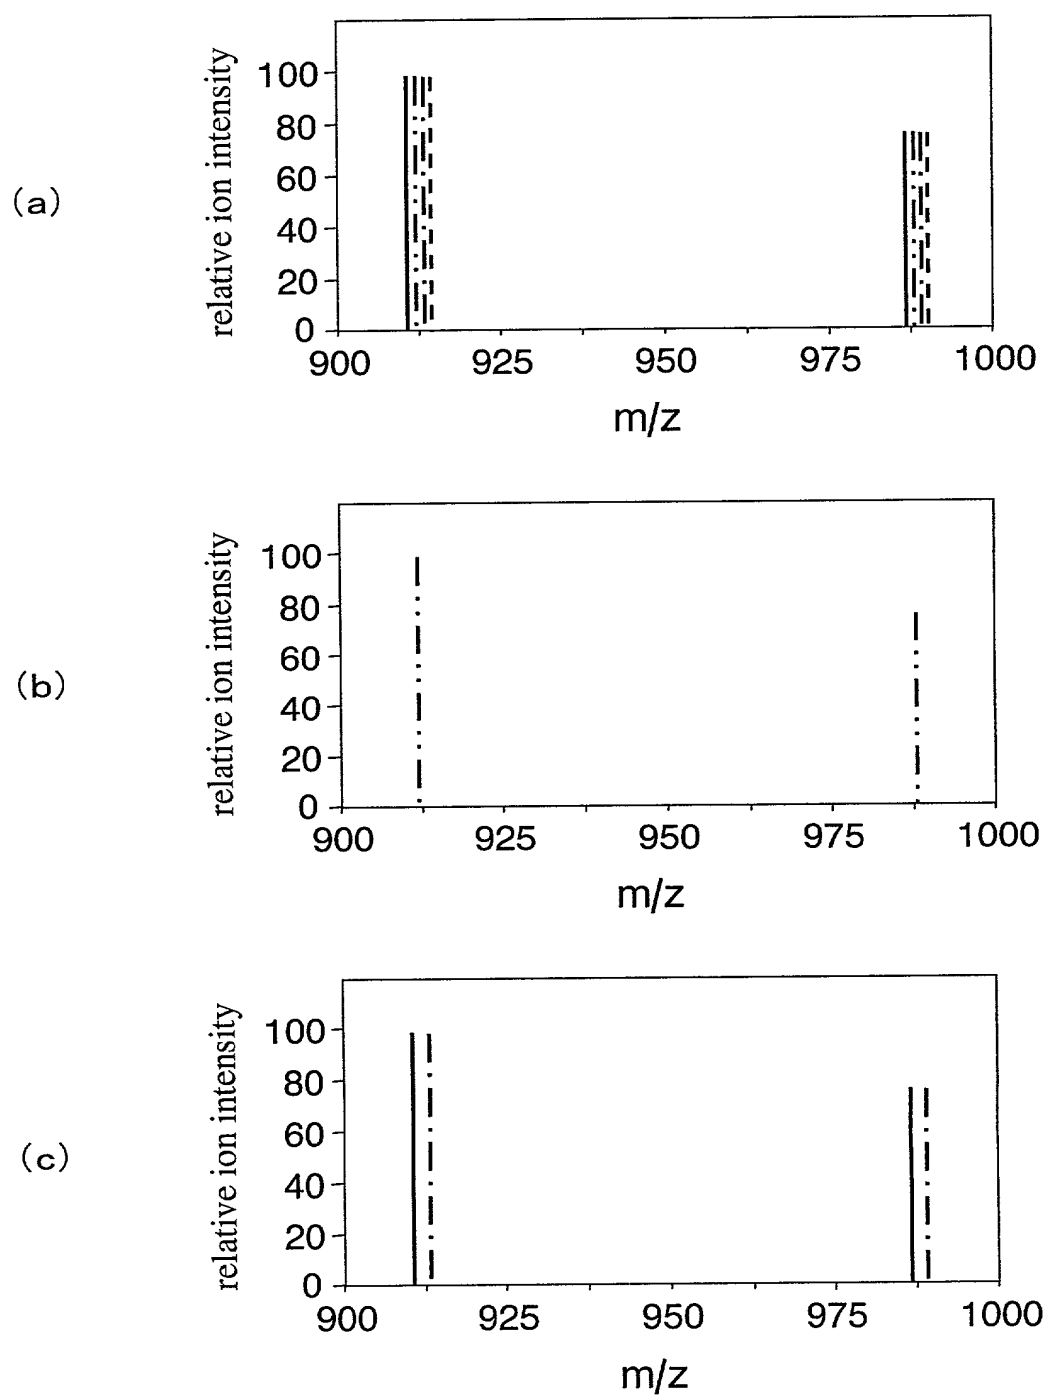


Fig. 6

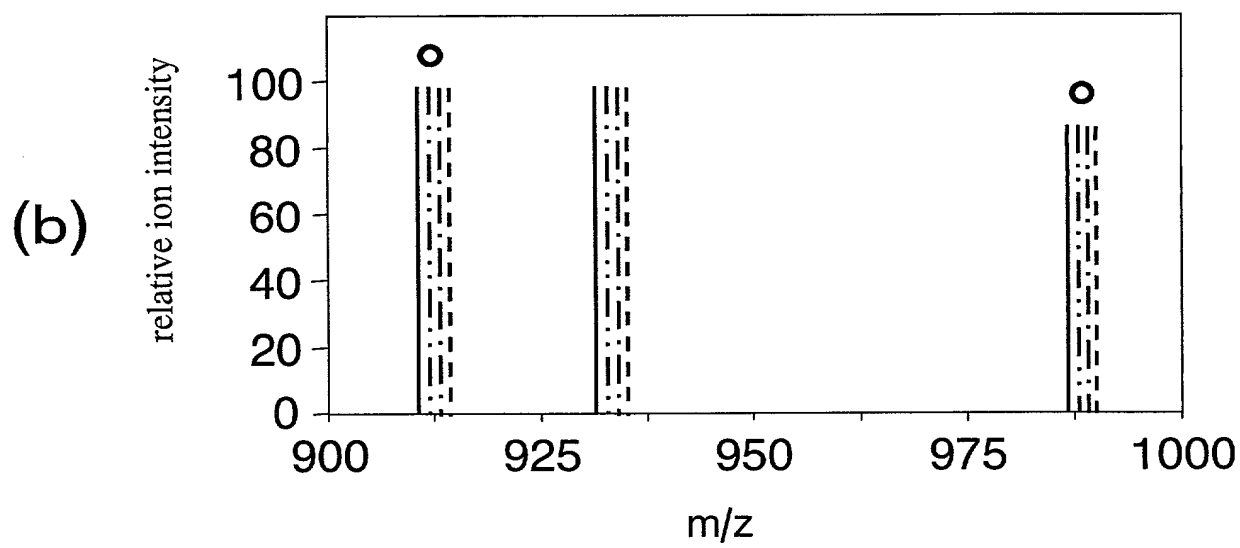
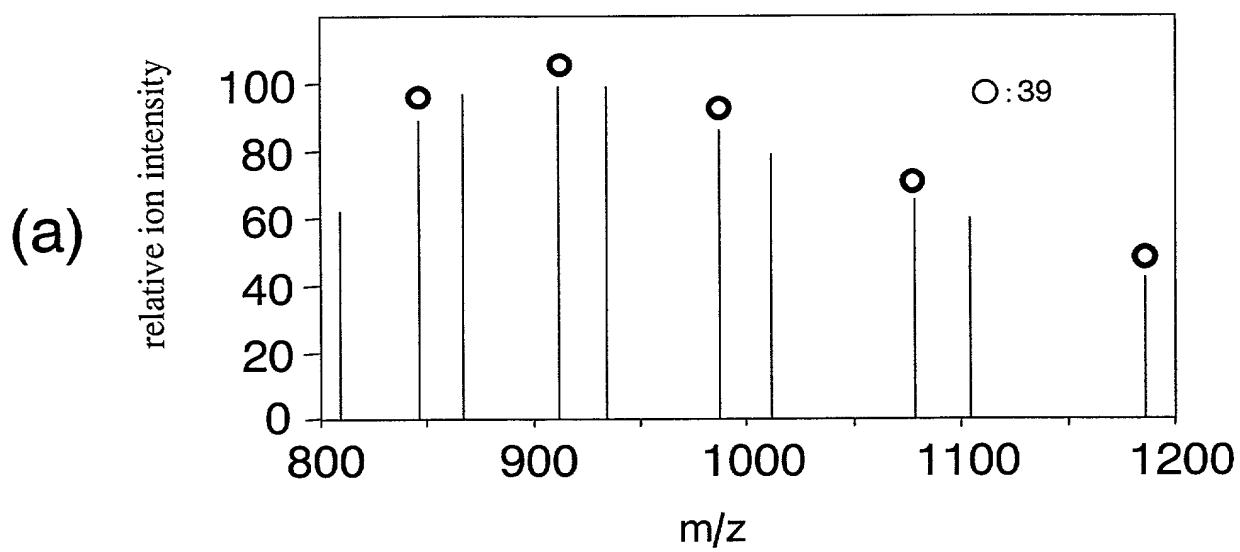


Fig. 7

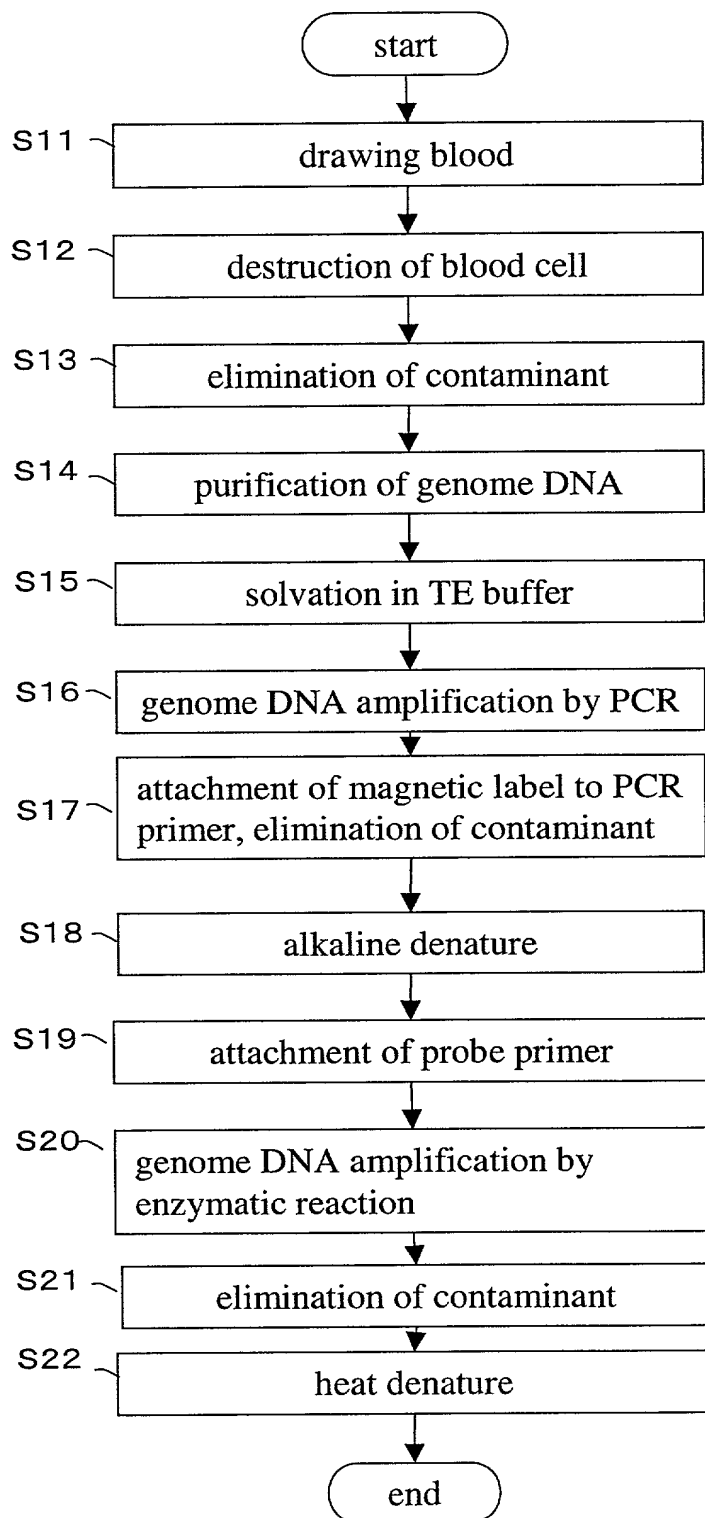


Fig. 8

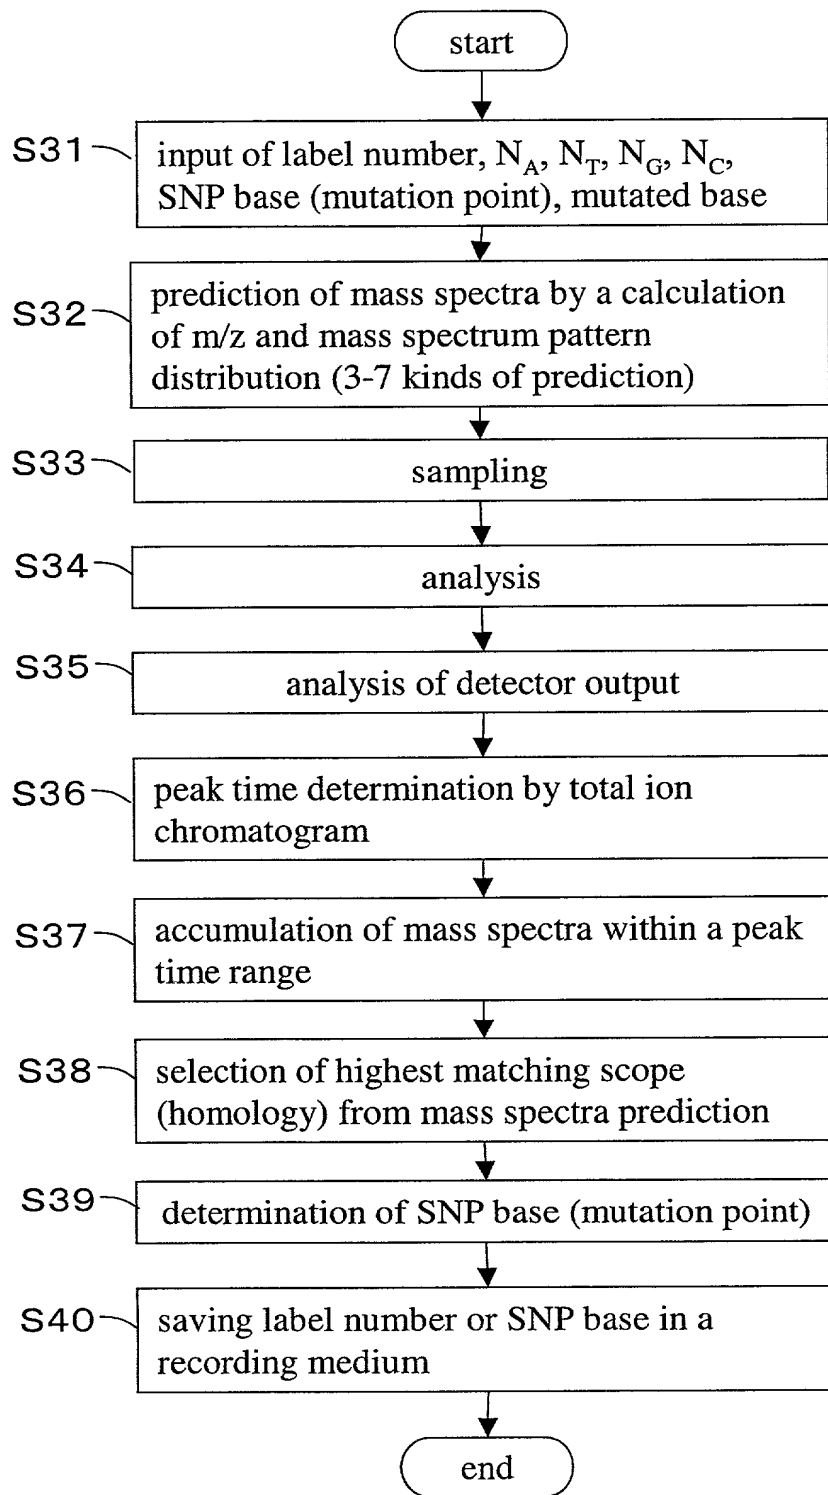


Fig. 9

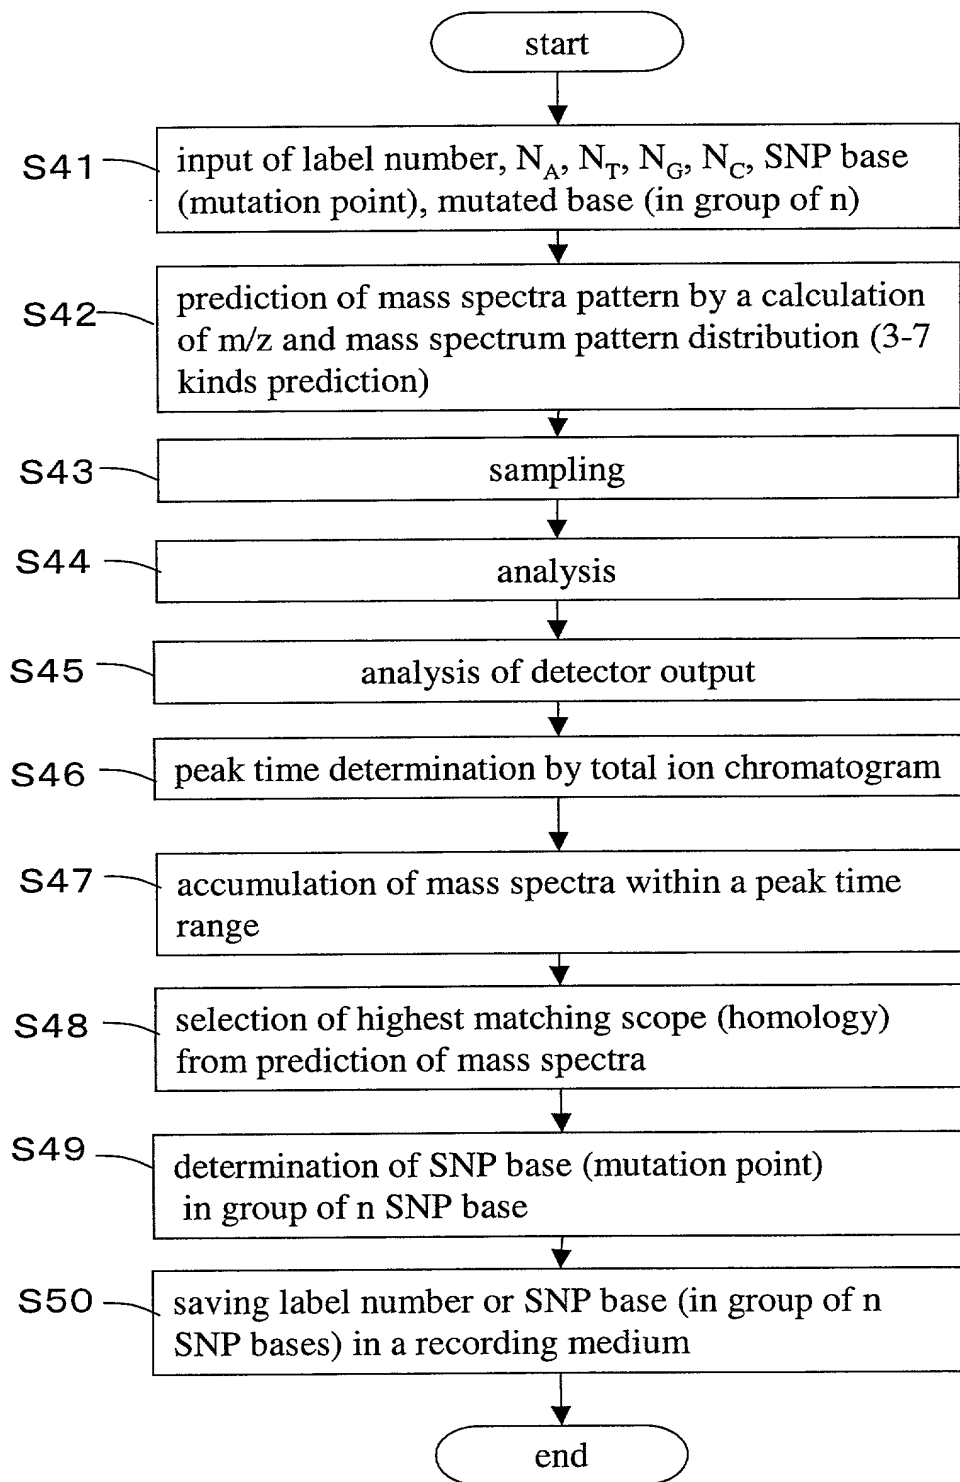


Fig. 10

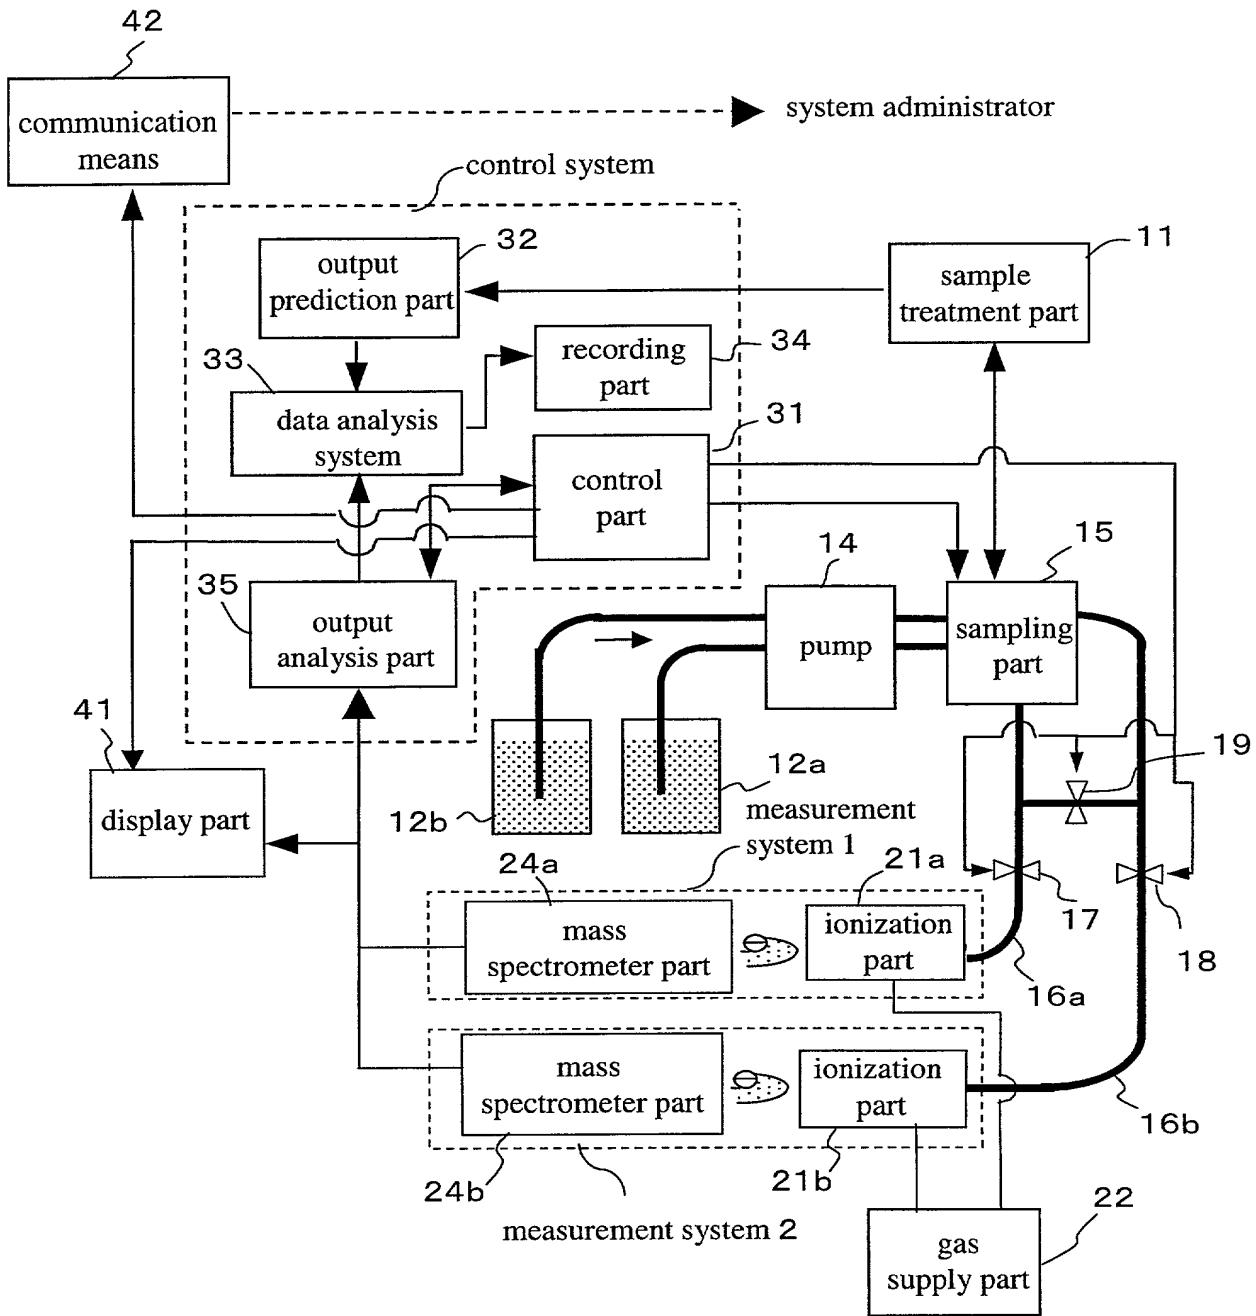


Fig. 11

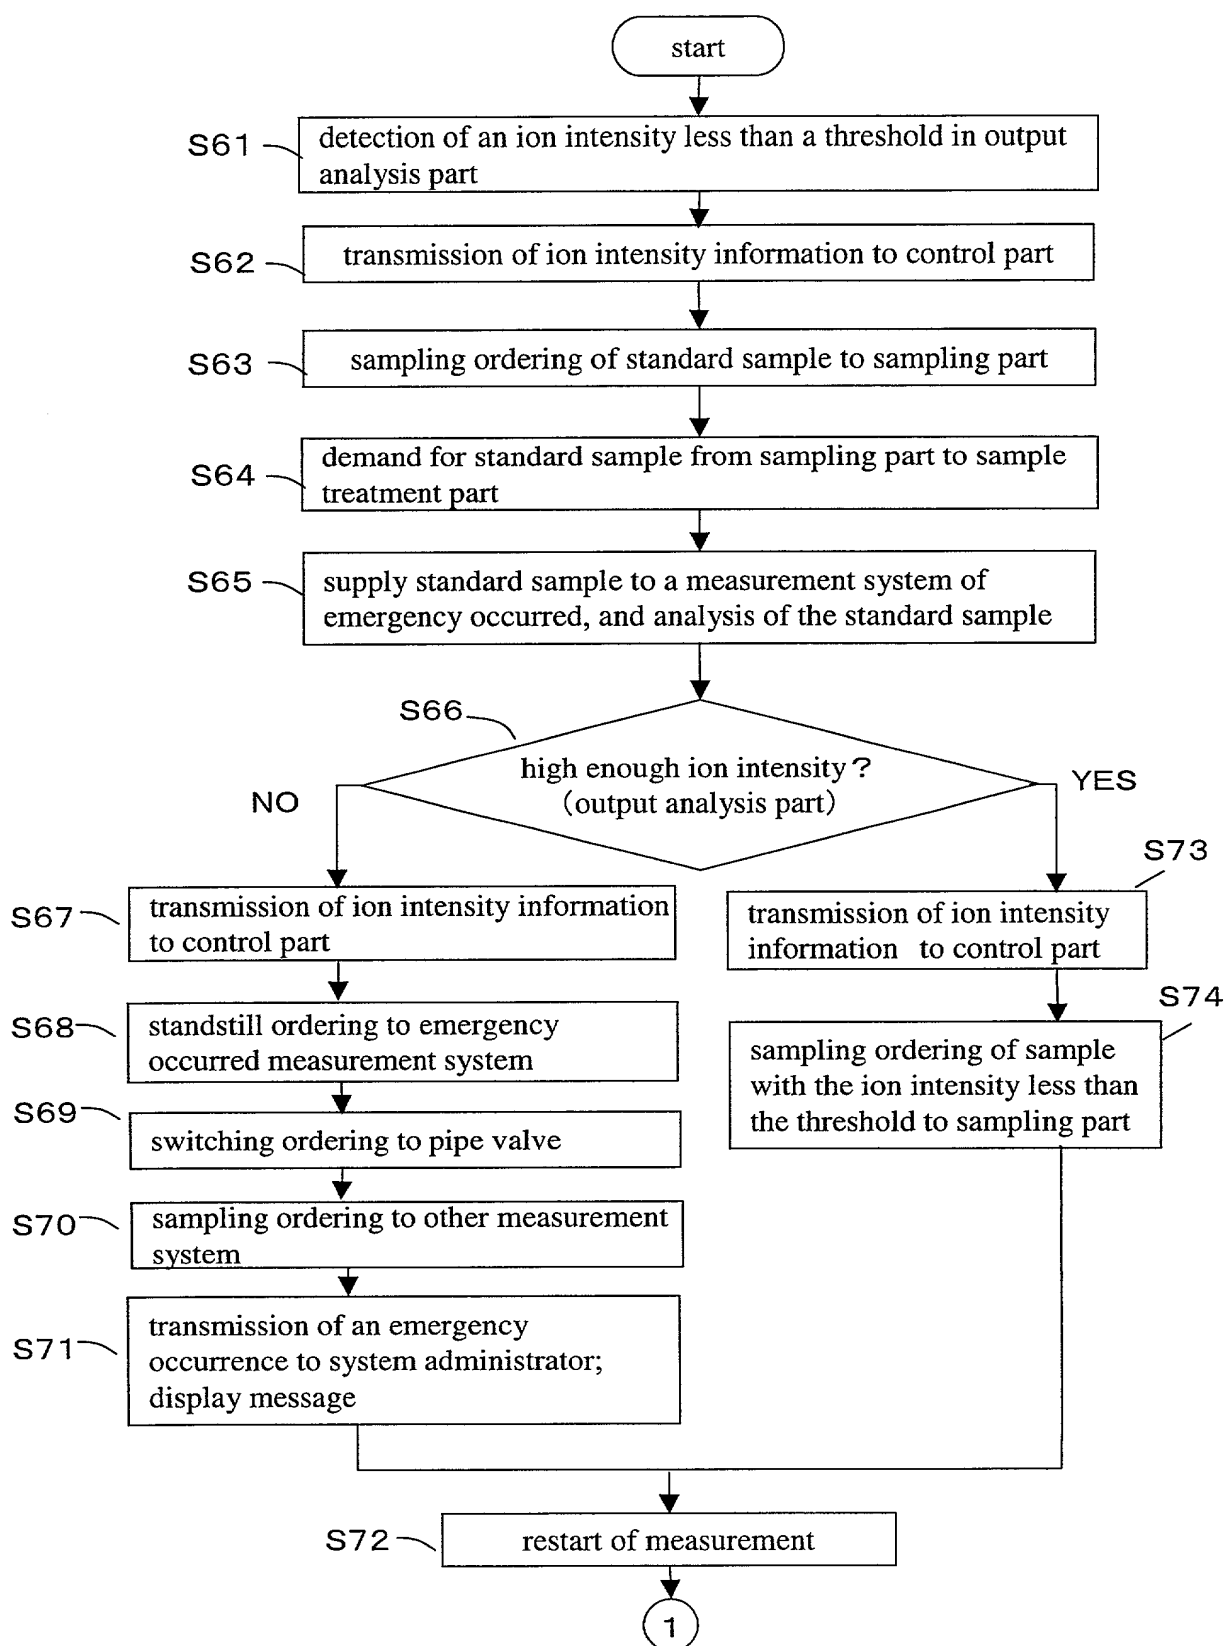


Fig. 12


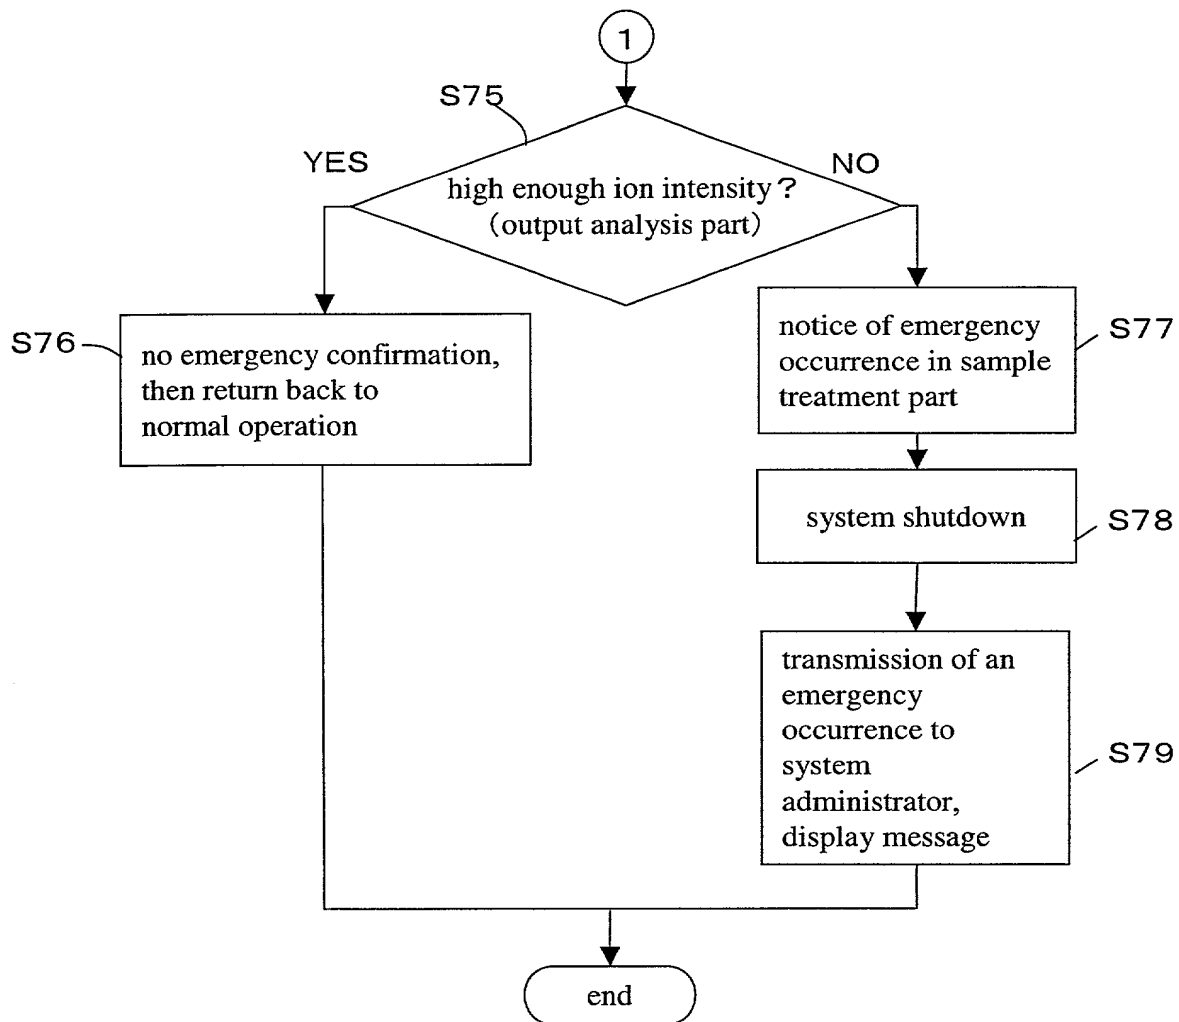


Fig. 13

status of analysis:  
normal

label number	base	notice
000814104853	A	
000814104854	A	
000814104855	A,T	
000814104856	A	
000814104857	A	
000814104858	A	
000814104859	T	
000814104900	A	
000814104901	A	

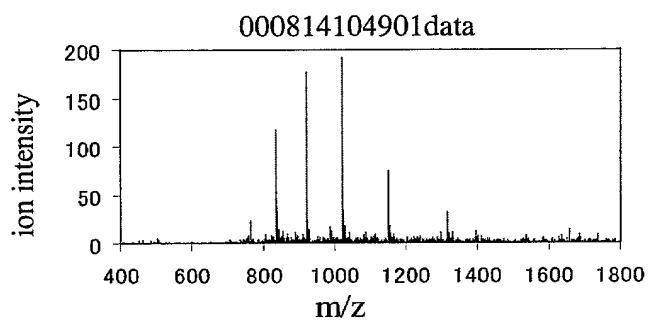

status of analysis:  
emergency shutdown

label number	base	notice
000814104853	A	
000814104854	A	
000814104855	A,T	
000814104856	A	
000814104857	A	
000814104858	A	
000814104859	T	
000814104900	?	
#####		standard sample

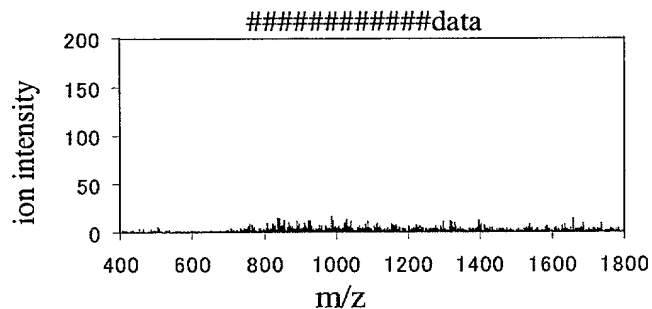


Fig. 14

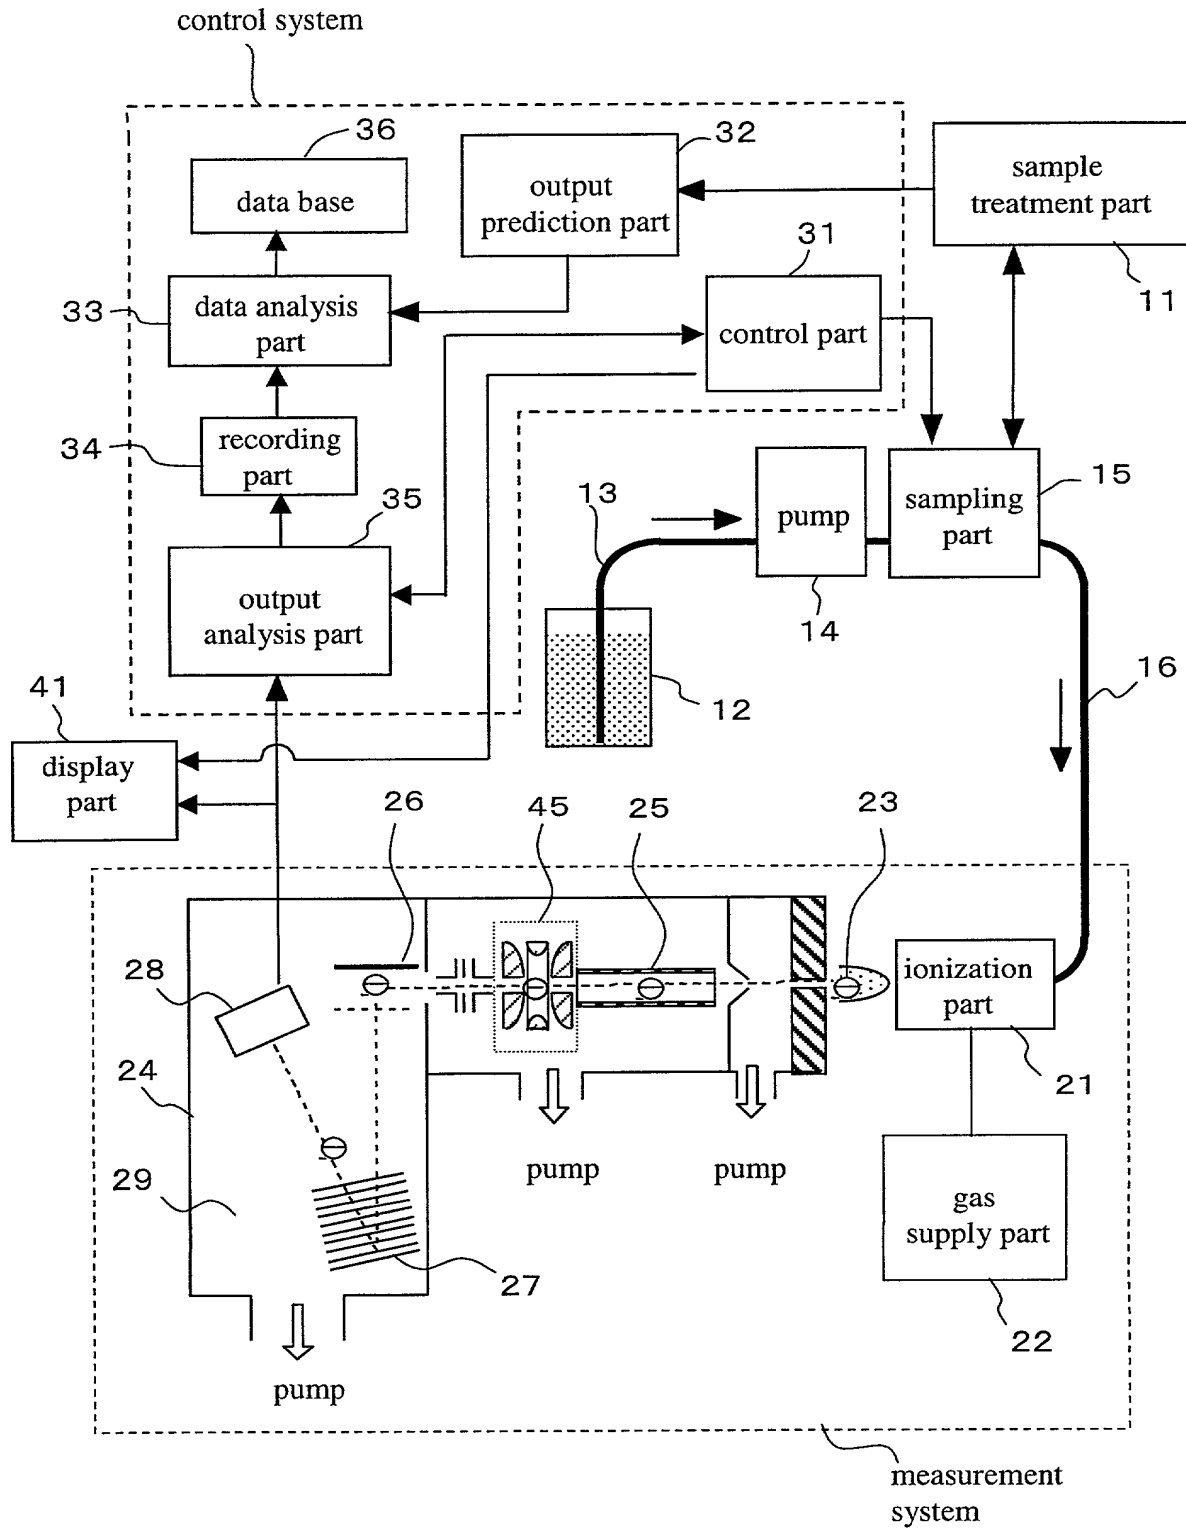


Fig. 15

